

Statistical and Fractal Processing of Phase Images of Human Biological Fluids

Yuriy USHENKO, Yuriy TOMKA, Yuriy MARCHUK, Valentine BALANETCKA
Chernivtsi National University, 58012, Chernivtsi, Ukraine
tomka.yuriy@gmail.com

Abstract—Performed in this work are complex statistical and fractal analyses of phase properties inherent to birefringence networks of liquid crystals consisting of optically-thin layers prepared from human bile. Within the framework of a statistical approach, the authors have investigated values and ranges for changes of statistical moments of the 1-st to 4-th orders that characterize coordinate distributions for phase shifts between orthogonal components of amplitudes inherent to laser radiation transformed by human bile with various pathologies. Using the Gramm-Charlie method, ascertained are correlation criteria for differentiation of phase maps describing pathologically changed liquid-crystal networks. In the framework of the fractal approach, determined are dimensionalities of self-similar coordinate phase distributions as well as features of transformation of logarithmic dependences for power spectra of these distributions for various types of human pathologies.

Index Terms—birefringence, biological fluid, correlation, Jones Matrix, liquid crystal, phase, polarization.

I. INTRODUCTION

Among the methods for optical diagnostics of human biological tissues (BT), the methods of laser polarimetric diagnostics aimed at their optically-anisotropic structure are widely spread [1 - 31]. The main “information product” of these methods is availability of coordinate distributions for azimuths $\alpha(x, y)$ and ellipticity $\beta(x, y)$ of polarization (polarization maps) with the following types of analyses: statistical (statistical moments of the 1-st to 4-th orders [5, 6, 10, 14, 19, 25, 26, 30]), correlation (auto- and joint correlation function [12, 17, 18, 21, 26]), fractal (fractal dimensionalities [5, 6, 25]), singular (distributions of amounts of linearly and circularly polarized states [22, 28]). As a result, interrelations between the set of these parameters and distributions of optical axis directions as well as values of the birefringence characterizing the network of optically uniaxial protein (myosin, collagen, elastin, etc.) fibrils in optically anisotropic components of BT layers can be determined. Using this base, developed is a set of methods for early recognition and differentiation of pathological changes in BT structures related with their degenerative-dystrophic and oncological changes [4-6, 12, 19, 20-22, 27, 29, 31].

It is noteworthy that there exists a widespread group of optically anisotropic biological objects for which the methods of laser polarimetric diagnostics are not so efficient. Optically-thin (coefficient of extinction $\tau \leq 0.1$) layers of various biological liquids (bile, urine, liquor,

synovial liquid, blood plasma, etc.) can be related to these objects. All these layers possess considerably less optical anisotropy of the biological component matter as compared with birefringent BT structures [4]. As a consequence, these objects weakly modulate polarization of laser radiation

($\begin{cases} \alpha(x, y) \approx const; \\ \beta(x, y) \rightarrow 0. \end{cases}$). On the other hand, the biological liquids

are more available for a direct laboratory analysis as compared to traumatic methods of BT biopsy. From the above reasoning, it seems topical to search new, additional parameters for laser diagnostics of optically anisotropic structures in biological liquids.

Our work is aimed at searching the possibilities to perform diagnostics of structures inherent to liquid-crystal networks of human bile with various pathologies by using the method to determine the coordinate distributions of phase shifts (phase maps) between orthogonal components of laser radiation amplitudes with the following statistical, correlation and fractal analyses of these distributions.

II. OPTICAL MODEL OF HUMAN BILE

As a base for modeling the optical properties of human bile we use the conception of anisotropy observed in BT protein networks developed in [1-4, 7, 9, 14, 16, 23-27, 30]:

human bile can be considered as a two-component amorphous-crystalline structure;

optically isotropic - optically homogeneous micellar solution;

optically anisotropic - liquid-crystalline phase, consisting of three types of liquid crystals: needle crystals of fatty acids, cholesterol monohydrate crystals, bilirubinate crystals of calcium.

The optical properties of amorphous $\{A\}$ and crystalline $\{C\}$ components of biological liquids can be exhaustively described using the following Jones operators [26]

$$\{A\} = \begin{vmatrix} a_{11} & a_{12} \\ a_{21} & a_{22} \end{vmatrix} = \begin{vmatrix} \exp(-\tau) & 0 \\ 0 & \exp(-\tau) \end{vmatrix}; \quad (1)$$

$$\{C\} = \begin{vmatrix} c_{11} & c_{12} \\ c_{21} & c_{22} \end{vmatrix} = \begin{vmatrix} \cos^2 \rho + \sin^2 \rho \exp(-i\delta) & \cos \rho \sin \rho [1 - \exp(-i\delta)] \\ \cos \rho \sin \rho [1 - \exp(-i\delta)] & \sin^2 \rho + \cos^2 \rho \exp(-i\delta) \end{vmatrix}. \quad (2)$$

Here, τ is the absorption coefficient for laser radiation in the biological liquid layer with the geometric thickness l ; ρ - direction of the optical axis; $\delta = 2\pi/\lambda \Delta n d$ - phase shift between the orthogonal components E_x and E_y of the amplitude of illuminating laser light with the wavelength λ ; Δn - index of birefringence.

The Jones matrix of the biological liquid layer, where isotropic and anisotropic creations lie in one plane, can be expressed as a sum of operators $\{A\}$ and $\{C\}$

$$\{M\} = \{A\} + \{C\} = \begin{pmatrix} a_{11} + c_{11} & a_{12} + c_{12} \\ a_{21} + c_{21} & a_{22} + c_{22} \end{pmatrix}, \quad (3)$$

Let us consider the process of transformation of the complex amplitude ($E \rightarrow U$) of a laser wave that passed through the biological liquid layer ($\{M\}$) located between two crossed phase filters – quarter-wave plates ($\{\Phi_1\}$ and $\{\Phi_2\}$) and polarizers ($\{P_1\}$ and $\{P_2\}$), planes of transmission for which make $+45^\circ$ and -45° angles with axes of the highest velocity. The amplitude U of the transformed laser beam in this experimental setup can be determined from the following matrix equation

$$U = 0.25 \{P_2\} \{\Phi_2\} \{M\} \{\Phi_1\} \{P_1\} E. \quad (4)$$

Here,

$$\left\{ \begin{array}{l} E = \begin{pmatrix} E_x \\ E_y \exp(-i\delta_0) \end{pmatrix}, \quad U = \begin{pmatrix} U_x \\ U_y \exp(-i\delta) \end{pmatrix}, \\ \{P_1\} = \begin{pmatrix} 1 & 1 \\ 1 & 1 \end{pmatrix}, \quad \{P_2\} = \begin{pmatrix} 1 & -1 \\ -1 & 1 \end{pmatrix}, \\ \{\Phi_1\} = \begin{pmatrix} 1 & 0 \\ 0 & i \end{pmatrix}, \quad \{\Phi_2\} = \begin{pmatrix} i & 0 \\ 0 & 1 \end{pmatrix}. \end{array} \right. \quad (5)$$

In the special case of a plane-polarized wave $E(E_x = E_y; \delta_0 = 0) = \begin{pmatrix} 1 \\ 1 \end{pmatrix}$, Eq. (4) acquires the look

$$U = 0.25 \begin{pmatrix} 1 & -1 \\ -1 & 1 \end{pmatrix} \begin{pmatrix} i & 0 \\ 0 & 1 \end{pmatrix} \times \begin{pmatrix} \cos^2 \rho + \sin^2 \rho \exp[-i\delta] & \cos \rho \sin \rho [1 - \exp[-i\delta]] \\ \cos \rho \sin \rho [1 - \exp[-i\delta]] & \sin^2 \rho + \cos^2 \rho \exp[-i\delta] \end{pmatrix} \times \begin{pmatrix} 1 & 0 \\ 0 & i \end{pmatrix} \begin{pmatrix} 1 \\ 1 \end{pmatrix} \quad (6)$$

The solution of the matrix equation (6) is the value of complex amplitude $U(\delta)$ that is determined exclusively by the phase shift δ and does not depend on orientation of the optical axis ρ for a laser image of biological liquid. Being based on it, one can write

$$I(\delta) = U U^* = I_0 \sin^2 \left[\frac{\delta}{2} \right]. \quad (7)$$

Here, I_0 is the intensity of a probing laser beam, $I_\delta(r)$ - intensity of the laser image for the biological liquid layer in the point (r) .

Interrelations (4) to (7) define the algorithm for direct experimental measuring the coordinate distribution of phase shifts $\delta(r)$ between orthogonal components of the amplitudes U_x, U_y in the laser image of an optically anisotropic biological liquid layer.

III. OPTICAL SCHEME AND METHOD FOR EXPERIMENTAL MEASURING THE PHASE MAPS OF BIOLOGICAL LIQUIDS

Shown in figure 1 is the optical scheme for phasometry of laser images obtained for biological liquids [4].

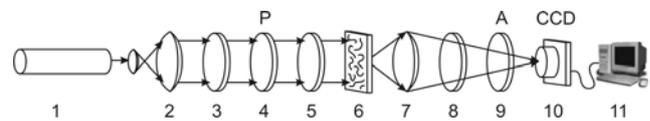


Figure 1. Optical scheme of the phase meter. 1 – He-Ne laser; 2 – collimator; 3, 5, 8 – quarter-wave plates; 4, 9 – polarizer and analyzer, respectively; 6 – investigated object; 7 – micro-objective; 10 – CCD camera; 11 – personal computer

Illumination was carried out using the parallel beam ($\varnothing = 10^4 \mu\text{m}$) of He-Ne laser 1 ($\lambda = 0.6328 \mu\text{m}$). Using the polarization illuminator (quarter-wave plate 3 and polarizer 4), we formed the beam linearly polarized with the azimuth 45° . The axis of the highest velocity of the quarter-wave plate 5 was oriented at the angle $\Theta = 45^\circ$ relatively to the transmission plane of the polarizer 4. Images of biological liquid layers 6 were projected using the micro-objective 7 into the plane of the light-sensitive area ($m \times n = 800 \text{ pix} \times 600 \text{ pix}$) of a CCD camera 10. Rotating the transmission plane of the analyzer 9 by the angle $\Theta = -45^\circ$ relatively to the axis of the highest velocity of the quarter-wave plate 8, formed were the conditions for transmission of left-circular polarized oscillations of points in laser images of biological liquids. The intensity of these oscillations I_δ was registered by each separate pixel in the CCD camera 10. Thus, we obtained the two-dimensional

$$\text{distribution } I_\delta \begin{pmatrix} r_{11} & \dots & r_{1n} \\ \dots & \dots & \dots \\ r_{m1} & \dots & r_{mn} \end{pmatrix} \text{ for this intensity. Further, in}$$

accord with (7), we calculated coordinate distributions (phase maps) for phase shifts $\delta(m \times n)$ between orthogonal components of the amplitude for laser images of biological liquids.

IV. ALGORITHMS FOR STATISTICAL, CORRELATION AND FRACTAL ANALYSES OF PHASE MAPS

To estimate $\delta(m \times n)$ distributions, we calculated the set of statistical moments of the 1-st to 4-th orders $M_{j=1,2,3,4}$ [5, 6, 25, 30]

$$\begin{aligned} M_1 &= \frac{1}{N} \sum_{i=1}^N |\delta_i|, & M_2 &= \sqrt{\frac{1}{N} \sum_{i=1}^N \delta_i^2}, \\ M_3 &= \frac{1}{M_2^3} \frac{1}{N} \sum_{i=1}^N \delta_i^3, & M_4 &= \frac{1}{M_2^4} \frac{1}{N} \sum_{i=1}^N \delta_i^4. \end{aligned} \quad (8)$$

As a base for the analysis of the coordinate structure of $\delta(m \times n)$, we took the autocorrelation method using the function [12, 21, 26]

$$K_{i=1 \div n}(\Delta m) = \lim_{m \rightarrow 0} \frac{1}{m} \int_1^m [\delta_i(m)] [\delta_i(m - \Delta m)] dm. \quad (9)$$

Here, $(\Delta m = 1 \text{ pix})$ is the step of changing the coordinate $(x = 1 \div m)$ of a distribution in the set of polarization distributions $\delta(m)$ for a specific i -th line. The overall expression for the autocorrelation function is obtained by averaging the expression (9) over all the lines $i = 1 \div n$

$$K(\Delta m) = \frac{\sum_{i=1}^n K_i(\Delta m)}{n}. \quad (10)$$

As correlation parameters that characterize the dependences $K(\Delta m)$, we used:

correlation area S

$$S = \int_1^m K(\Delta m) dm, \quad (11)$$

normalized fourth statistical moment Q_4 that determine the excess of the autocorrelation function $K(\Delta m)$

$$Q_4 = \frac{N}{\left(\sum_{i=1}^N (K(\Delta m))_i^2 \right)^2} \sum_{i=1}^N (K(\Delta m))_i^4; \quad (12)$$

The fractal analysis of $\delta(m \times n)$ distributions was performed using the calculation of logarithmic dependences $\log J(\delta) - \log d^{-1}$ for the power spectra $J(\delta)$

$$J(\delta) = \int_{-\infty}^{+\infty} \delta \cos 2\pi \nu d \nu, \quad (13)$$

where $\nu = d^{-1}$ are spatial frequencies that are determined by geometrical dimensions (d) inherent to structural

elements of laser images for biological liquids.

The dependences $\log J(\delta) - \log d^{-1}$ are approximated using the least-squares method into the curves $V(\eta)$, straight parts of which are used to determine the slope angles η and fractal dimensionalities F in accord with the relation [5, 6, 11, 25]

$$F = 3 - \text{tg } \eta. \quad (14)$$

Classification of coordinate $\delta(m \times n)$ distributions is fulfilled using the following criteria:

they are fractal with the proviso that the slope angle is constant ($\eta = \text{const}$) for 2 – 3 decades of changing the sizes d ;

they are multi-fractal on the condition that there available are several slope angles $V(\eta)$;

they are random, if any stable slope angles $V(\eta)$ do not exist within the whole range of changing the sizes d .

In the latter case, the $\log J(\delta) - \log d^{-1}$ distributions are characterized with the dispersion

$$D = \sqrt{\frac{1}{N} \sum_{i=1}^N [\log J(\delta) - \log d^{-1}]^2} \quad (15)$$

V. STATISTICAL, CORRELATION AND FRACTAL PARAMETERS OF PHASE MAPS FOR HUMAN BILE

As objects for experimental studying, we chose optically-thin layers of synovial liquid taken from a healthy patient (figure 2a) and with atrophic arthritis (figure 2b).

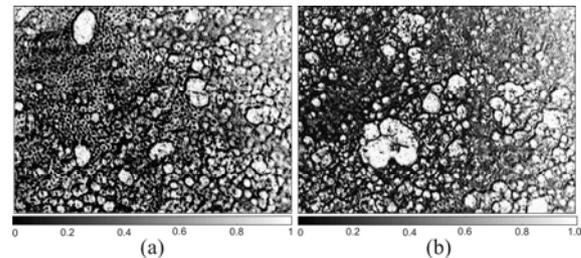


Figure 2. Polycrystalline networks of human bile taken from healthy patient (a) and patient suffering from diabetes of 2nd level (b).

The images of layers prepared from human bile (figure 2) are indicative of availability of two fractions – optically isotropic and liquid-crystal network (anisotropic one). As seen, geometric structure and sizes of separate elements in the polycrystalline network of the samples prepared from biological liquids are individual for physiological state.

Shown in figure 3 are the phase maps (fragments (a), (b), (c), (d)) and histograms (fragments (e), (f)) for distributions of random values inherent to the phase shifts δ between orthogonal components of the laser radiation amplitude transformed inside layers of synovial liquid taken from healthy patient's (left column) and from patient suffering from diabetes of 2nd level (right column).

The obtained data show that the value of phase shifts δ for laser radiation transformed inside layers of human bile lies within the short range of changes $0 \leq \delta \leq \pi$. The weak

phase modulation is related with two factors. First, it is low geometric thickness ($d = 10 \dots 15 \mu\text{m}$) of the samples. Second, it is weak birefringence ($\Delta n \sim 10^{-4} \dots 10^{-2}$) of liquid-crystal structures in human bile.

Our comparative analysis of histograms for distributions of random values inherent to phase shifts δ in laser images of both types human bile revealed availability of two dominant extreme ranges: $0 \leq \delta \leq 0.15$ and $0.85 \leq \delta \leq 1$. In our opinion, these features of probabilistic phase distributions are related with the influence of optically isotropic ($\delta \rightarrow 0$) and liquid-crystal ($\delta \rightarrow \pi$) components in the composition of biological liquid.

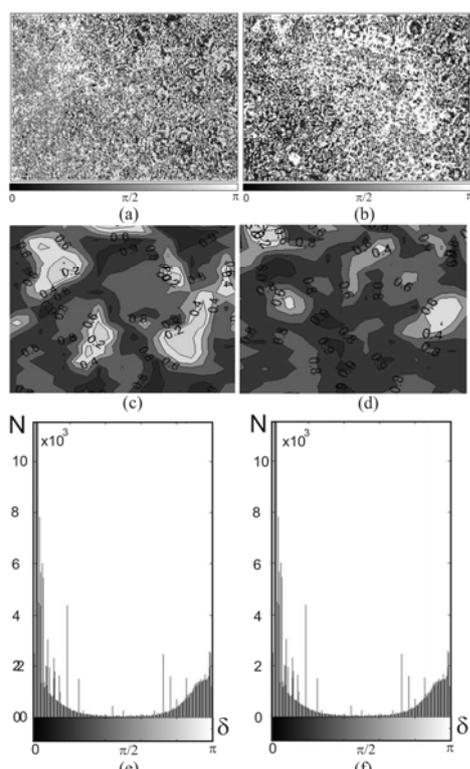


Figure 3. Coordinate (a, b) and quantitative (c, d) distributions δ of laser images for the samples of bile synovial liquid taken from healthy patient's (a, c, e) and with diabetes of 2nd level (b, d, f).

Table 1 contains data on the value of statistical moments of 1st – 4th order, which characterize the distribution of phase shifts of bile laser images of two groups of healthy ($q = 21$) and ill patients ($q = 19$).

TABLE 1. STATISTICAL MOMENTS $R_{i=1-4}^\delta$ OF PHASE COORDINATE DISTRIBUTION $\delta(x, y)$ OF LASER RADIATION WHICH IS TRANSFORMED BY SAMPLES OF BILE TAKEN FROM HEALTHY PATIENT AND PATIENT SUFFERING FROM DIABETES OF 2ND LEVEL

$R_{i=1-4}^\delta$	Healthy (21 patients)	Diabetes (19 patients)
R_1^δ	$0,25 \pm 0,032$	$0,28 \pm 0,035$
R_2^δ	$0,36 \pm 0,045$	$0,31 \pm 0,042$
R_3^δ	$0,83 \pm 0,092$	$0,77 \pm 0,081$
R_4^δ	$0,47 \pm 0,058$	$0,56 \pm 0,067$

The results show that the differentiation phase maps of different groups is impossible - change of size and range of statistical moments of 1 - 4-th order almost coincide.

Being aimed at more specific investigation of phase features for both fractions, we used the following method to select information. From the available coordinate set of values $\delta(m \times n) = \begin{pmatrix} \delta_{11}, \dots, \delta_{1n} \\ \delta_{n1}, \dots, \delta_{nn} \end{pmatrix}$ in phase maps (figures 3(a) and 3(b)), we found samples of extreme values $\delta(m \times n) = 0$ and $\delta(m \times n) = \pi$. In what follows, by scanning along the direction $x = 1 \div n$ we carried out calculation of the amount of extreme values for phase shifts within the column $m = n \times 1 \text{ pix}$. Within the limits of each local sample $(1_{\text{pix}} \times n_{\text{pix}})^{(k=1,2,\dots,m)}$, we computed the amount (N) of extreme values $\delta(k) = 0$ ($N_{\text{min}}^{(k)}$) and $\delta(k) = \pi$ ($N_{\text{max}}^{(k)}$). Thus, we found the dependences $N_{\text{msn}}(x) \equiv (N_{\text{msn}}^{(1)}, N_{\text{min}}^{(2)}, \dots, N_{\text{min}}^{(m)})$ and $N_{\text{max}}(x) \equiv (N_{\text{max}}^{(1)}, N_{\text{max}}^{(2)}, \dots, N_{\text{max}}^{(m)})$ for the amount of extreme values of phase shifts within the limits of laser image for bile.

Figures 4 and 5 show a set of coordinate distributions $\delta(m \times n) = 0, \pi$ (fragments (a, e)) for the dependences of the amount of extreme values $N_{\text{min,max}}(x)$ (fragments (b, f)), autocorrelation functions $K_{\text{min,max}}(\Delta x)$ (fragments (c, g)) and logarithmic dependences $\log J(N_{\text{min,max}}) - \log d^{-1}$ for power spectra of distributions $N_{\text{min,max}}(x)$ (fragments (d, h)) that characterize phase maps for the samples of synovial liquid belonging to a healthy patient (left column) and a patient suffering from diabetes of 2nd level (right column).

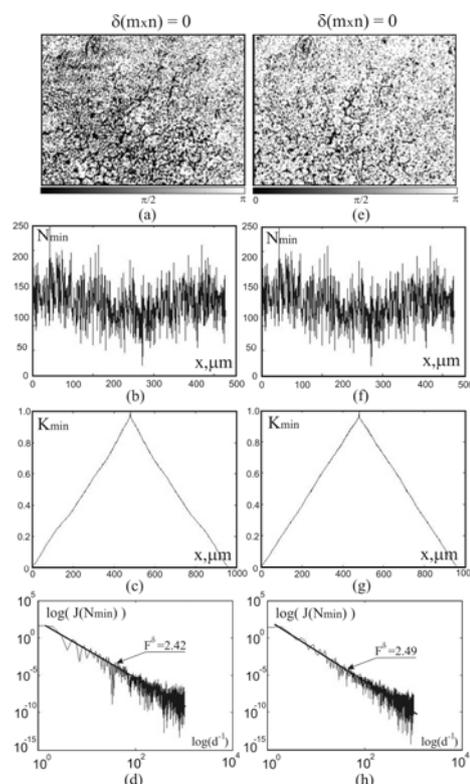


Figure 4. Coordinate ($m \times n$) (a, e), quantitative $N_{\text{min}}(x)$ (b, f), correlation $K_{\text{min}}(\Delta x)$ (c, g) and fractal $\log J(N_{\text{min}}) - \log d^{-1}$ (d, h) parameters of the extreme sample $\delta(m \times n) = 0$ for phase maps of the samples of ble belonging to a healthy patient (a, b, c, d) and a patient with diabetes of 2nd level (e, f, g, h).

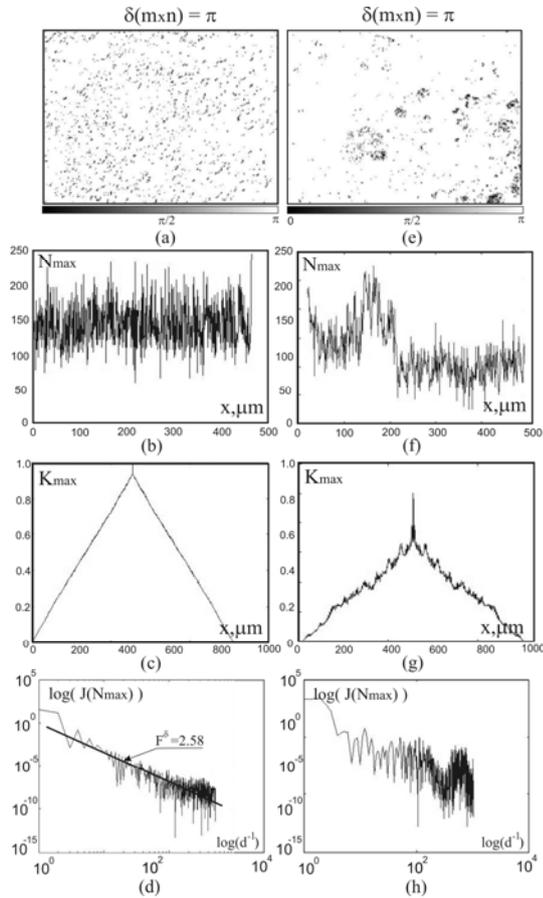


Figure 5. Coordinate $(m \times n)$ (a, e), quantitative $N_{\max}(x)$ (b, f), correlation $K_{\max}(\Delta x)$ (c, g) and fractal $\log J(N_{\max}) - \log d^{-1}$ (d, h) parameters of the extreme sample $\delta(m \times n) = 1$ for phase maps of the samples of bile belonging to a healthy patient (a, b, c, d) and a patient with diabetes of 2nd level (e, f, g, h).

The comparative analysis of the obtained set of experimental data about statistical, correlation and fractal structures in dependences for the amount of extreme values $N_{\min, \max}(x)$ inherent to phase maps describing layers of bile of healthy patient and that sick with diabetes of 2nd level enabled to found:

- tendency to a decreasing (increasing) total amount of extreme values $\delta_{\min} \rightarrow 0$ ($\delta_{\max} \rightarrow \pi$) of the phase shifts in laser images of layers prepared from bile of a patient with diabetes of 2nd level (figures 4 and 5, fragments (b, f));
- fact that autocorrelation functions $K_{\min}(\Delta x)$ (figure 4, fragments (c, g)) monotonically drop with increasing the step of scanning Δx in dependences $N_{\min}(x)$;
- correlation structure of the distribution for the extreme sample $\delta(m \times n) = \pi$ in the phase map describing the polycrystalline component in bile of a sick patient changes: at the background of monotonic drop there arise oscillations of values in the dependence $K_{\max}(\Delta x)$ (see figure 5, fragment (g));
- logarithmic dependences for the power spectra of distributions $N_{\min}(x)$ for the optically isotropic component in bile of both types possess a stable slope angle (figure 4, fragments (d, f)) within the whole range of geometric sizes inherent to the laser image registered by the CCD camera (figure 1);

- fractal distributions $N_{\max}(x)$ for phase maps of laser images describing the optically anisotropic fraction of bile a healthy man (figure 5, fragment (d)) are transformed into the statistical ones in the case of diabetes of 2nd level: approximating curve in the dependence $\log J(N_{\max}) - \log d^{-1}$ has no stable slope (Fig. 5, fragment (h)).

From the quantitative viewpoint, the dependences $N_{\min, \max}(x)$ illustrate statistical $M_{i=1-4}^\delta$, correlation $R^\delta, S^\delta, Q^\delta$ and fractal F^δ, D^δ parameters determined within the limits of two patient groups, and they are summarized in Tables 2.

Our analysis of the parameters determined experimentally has shown that the following parameters are diagnostically sensitive in observation of inflammatory processes

- statistical moments of the third (M_3^δ) and fourth (M_4^δ) orders in distributions for the amount of extreme values $N_{\max}(x)$ of phase shifts $\delta(m \times n) = 1$ in laser images for bile of both types – differences between them reach 2.4 and 4.1 times;
- excess (R_4^δ) of autocorrelation functions $K_{\max}(\Delta x)$ related to distributions $N_{\max}(x)$ differ by 1.8 and 2.7 times;

TABLE 2. STATISTICAL MOMENTS $M_{i=1-4}^\delta$, CORRELATION $R^\delta, S^\delta, Q^\delta$ AND FRACTAL F^δ, D^δ PARAMETERS THAT CHARACTERIZE THE DISTRIBUTIONS FOR AMOUNTS OF EXTREME VALUES IN COORDINATE DISTRIBUTIONS $\delta(m \times n)$ OF LASER IMAGES FOR HUMAN BILE

$\delta(m \times n)$	$\delta(m \times n) = 0$		$\delta(m \times n) = \pi$	
	Healthy (21 patients)	Diabetes (19 patients)	Healthy (21 patients)	Diabetes (19 patients)
$M_{i=1-4}^\delta$				
M_1^δ	0.51±0.063	0.54±0.067	0.22±0.025	0.35±0.042
M_2^δ	0.13±0.018	0.08±0.011	0.25±0.031	0.14±0.017
M_3^δ	0.26±0.033	0.19±0.022	0.79±0.086	2.18±0.25
M_4^δ	0.48±0.054	0.55±0.068	0.83±0.098	3.11±0.42
R_4^δ	0.14±0.016	0.12±0.015	0.56±0.069	2.21±0.31
S^δ	0.24±0.015	0.21±0.013	0.17±0.021	0.08±0.012
F^δ	2.42±0.12	2.49±0.11	2.58±0.15	Statistical
D^δ	0.21±0.028	0.24±0.027	0.34±0.042	0.18±0.023

- correlation area S^δ for the autocorrelation dependence $K_{\max}(\Delta x)$ of the distribution for the amount of extreme phase shifts in a laser image inherent to joint bile of a patient with osteoarthritis is 2.55 times less than that parameter determined for a healthy patient;
- distributions $N_{\max}(x)$ for the phase maps describing bile for healthy and sick patients are, respectively, fractal and statistical;
- dispersion D^δ of the dependences $\log J(N_{\max}) - \log d^{-1}$ in the case of pathological changes in the polycrystalline structure of bile is 1.75 times decreased.

VI. CONCLUSIONS

Thus, one can draw the following conclusions:

➤ Human bile, independently of their physiological state, contains phase-modulating optically anisotropic network of biological crystals.

➤ Ascertained and grounded is a set of criteria for phase diagnostics of inflammatory processes (diabetes, cholecystitis) as being based on statistical (statistical moments of the first to fourth orders), correlation (statistical moments for the Gramm-Charlie expansion, correlation area) and fractal (fractal dimensionality and dispersion for the distribution of extrema in log – log dependences of power spectra) analyses of phase distributions in laser images of human bile.

REFERENCES

- [1] W.-F. Cheong, S. A. Pahl, A. J. Welch, "A Review of the Optical Properties of Biological Tissues," *IEEE J. Quantum Electron*, Vol. 26, pp. 2166-2185, Dec. 1990.
- [2] S. A. Pahl, M. Keijzer, S. L. Jacques, A. J. Welch, "A Monte Carlo model of light propagation in tissue," *SPIE Proceedings of Dosimetry of Laser Radiation in Medicine and Biology*, Vol. IS 5, pp. 102-111, 1989.
- [3] E. Wolf, "Unified theory of coherence and polarization of random electromagnetic beams," *Phys. Lett. A*, Vol. 312, pp. 263-267, 2003.
- [4] Alexander G. Ushenko and Vasilii P. Pishak, "Laser Polarimetry of Biological Tissue: Principles and Applications", in *Handbook of Coherent-Domain Optical Methods: Biomedical Diagnostics, Environmental and Material Science*, vol. I, Valery V. Tuchin, Ed. Boston: Kluwer Academic Publishers, 2004, pp. 93-138.
- [5] O. V. Angelsky, A. G. Ushenko, Yu. A. Ushenko, V. P. Pishak, "Statistical and Fractal Structure of Biological Tissue Mueller Matrix Images", in *Optical Correlation Techniques and Applications*, Oleg V. Angelsky, Ed. Washington: Society of Photo-Optical Instrumentation Engineers, 2007, pp. 213-266.
- [6] O.V. Angelsky, A.G. Ushenko, Yu.A. Ushenko, V.P. Pishak, and A.P. Peresunko, "Statistical, Correlation, and Topological Approaches in Diagnostics of the Structure and Physiological State of Birefringent Biological Tissues", in *Handbook of Photonics for Biomedical Science*, Valery V. Tuchin, Ed. USA: CRC Press, 2010, pp. 21-67.
- [7] Alexander G. Ushenko, "Polarization structure of laser scattering fields," *Optical Engineering*, vol. 34(4), pp. 1088-1093, November 1995.
- [8] A.G. Ushenko, "Laser diagnostics of biofractals," *Quantum Electronics*, vol. 29(12), pp. 1078-1084, December 1999.
- [9] O.V. Angel'skii, A.G. Ushenko, A.D. Arkhelyuk, S.B. Ermolenko, D.N. Burkovets, "Structure of matrices for the transformation of laser radiation by biofractals," *Quantum Electronics*, vol. 29(12), pp. 1074-1077, December 1999.
- [10] O.V. Angel'skii, A.G. Ushenko A.D. Arheluk, S.B. Ermolenko, D. N. Burkovets, "Scattering of Laser Radiation by Multifractal Biological Structures," *Optics and Spectroscopy*, vol. 88(3), pp. 444-448, March 2000.
- [11] A.G. Ushenko, "Polarization Structure of Biospeckles and the Depolarization of Laser Radiation," *Optics and Spectroscopy*, vol. 89(4), pp. 597-601, October 2000.
- [12] A.G. Ushenko, "Stokes-correlometry of biotissues," *Laser Physics*, vol. 10(5), pp.1286-1292, May 2000.
- [13] A.G. Ushenko, "The Vector Structure of Laser Biospeckle Fields and Polarization Diagnostics of Collagen Skin Structures," *Laser Physics*, vol. 10(5), pp. 1143-1149, May 2000.
- [14] A.G. Ushenko, "Laser polarimetry of polarization-phase statistical moments of the object field of optically anisotropic scattering layers," *Optics and Spectroscopy*, vol. 91(2), pp. 313-316, February 2001.
- [15] A.G. Ushenko, "Polarization contrast enhancement of images of biological tissues under the conditions of multiple scattering," *Optics and Spectroscopy*, vol. 91(6), pp. 937-940, August 2001.
- [16] A.G. Ushenko, "Laser probing of biological tissues and the polarization selection of their images," *Optics and Spectroscopy*, vol. 91(6), pp.932-936, August 2001.
- [17] A.G. Ushenko, "Correlation processing and wavelet analysis of polarization images of biological tissues," *Optics and Spectroscopy*, vol. 91(5), pp.773-778, June 2002.
- [18] A.G. Ushenko, "Polarization correlometry of angular structure in the microrelief pattern or rough surfaces," *Optics and spectroscopy*, vol. 92(2), pp. 227-229, June 2002.
- [19] O.V. Angelsky, A.G. Ushenko, Ye.G. Ushenko, "2-D Stokes Polarimetry of Biospeckle Tissues Images in Pre-Clinic Diagnostics of Their Pre-Cancer States," *Journal of Holography and Speckle*, vol. 2(1), pp. 26-33, April 2005.
- [20] Oleg V. Angelsky, Alexander G. Ushenko, and Yevheniya G. Ushenko, "Complex degree of mutual polarization of biological tissue coherent images for the diagnostics of their physiological state," *J. Biomed. Opt.*, vol. 10(6), Article ID 060502, November 2005.
- [21] O. V. Angelsky, A. G. Ushenko, and Ye. G. Ushenko, "Investigation of the correlation structure of biological tissue polarization images during the diagnostics of their oncological changes," *Physics in Medicine and Biology*, vol. 50(20), pp. 4811-4822, September 2005.
- [22] Oleg V. Angelsky, Alexander G. Ushenko, Yevheniya G. Ushenko, Yuriy Y. Tomka, "Polarization singularities of biological tissues images," *J. Biomed. Opt.*, vol. 11(5), Article ID 054030, September-October 2006.
- [23] O.G. Ushenko, S.G. Guminetsky, A.V. Motrich, "Optical properties of urine, blood plasma and pulmonary condensate of the patients with pulmovnary form of tuberculosis," *Photoelectronics*, vol.16, pp. 133-139, June 2007.
- [24] S.H. Guminetskiy, O.G. Ushenko, I.P. Polyanskiy, A.V. Motrych, F.V. Grynchuk, "The optical method for investigation of the peritonitis progressing process," *Proceedings of the SPIE*, vol. 7008, Article ID 700827, April 2008.
- [25] Alexander Ushenko, Sergej Yermolenko, Alexander Prydij, Stepan Guminetsky, Ion Gruia, Ovidiu Toma, Konstantin Vladychenko, "Statistical and fractal approaches in laser polarimetry diagnostics of the cancer prostate tissues," *Proceedings of the SPIE*, vol. 7008, Article ID 70082C, April 2008.
- [26] A.G. Ushenko, A.I. Fediv, Yu.F. Marchuk, "Correlation and fractal structure of Jones matrices of human bile secret," *Proceedings of the SPIE*, vol. 7368, Article ID 73681Q, July 2009.
- [27] A.G. Ushenko, Yu.Ya. Tomka, V.I. Istratiy, "Polarization selection of two-dimensional phase-inhomogeneous birefringence images of biotissues," *Proceedings of the SPIE*, vol. 7388, Article ID 73881L, December 2009.
- [28] A.G. Ushenko, A.I. Fediv, Yu.F. Marchuk, "Singular structure of polarization images of bile secret in diagnostics of human physiological state," *Proceedings of the SPIE*, vol. 7368, Article ID 73681S, July 2009.
- [29] S.B. Yermolenko, A.G. Ushenko, P. Ivashko, "Spectropolarimetry of cancer change of biotissues," *Proceedings of the SPIE*, vol. 7388, Article ID 73881D, December 2009.
- [30] A.G. Ushenko, I. Z.Misevich, V. Istratiy, I. Bachyns'ka, A. P. Peresunko, Omar Kamal Numan, and T. G. Moiyusuk, "Evolution of Statistic Moments of 2D-Distributions of Biological Liquid Crystal Net Mueller Matrix Elements in the Process of Their Birefringent Structure Changes," *Advances in Optical Technologies*, vol. 2010, Article ID 423145, March 2010.
- [31] O. V. Dubolozov, A. G. Ushenko, V. T. Bachynsky, A. P. Peresunko, and O. Ya. Vanchulyak, "On the Feasibilities of Using the Wavelet Analysis of Mueller Matrix Images of Biological Crystals," *Advances in Optical Technologies*, vol. 2010, Article ID 162832, March 2010